






World Health
Organization

unicef 
for every child

WHO-UNICEF TECHNICAL SPECIFICATIONS AND GUIDANCE FOR OXYGEN THERAPY DEVICES

WHO MEDICAL DEVICE TECHNICAL SERIES

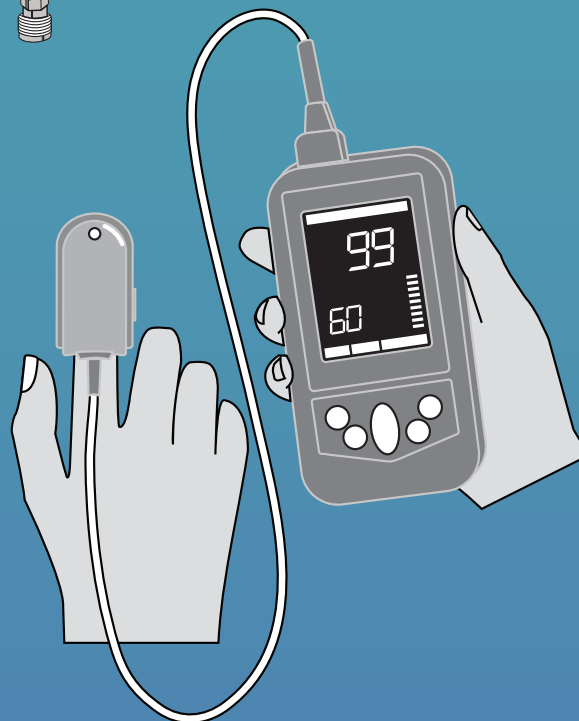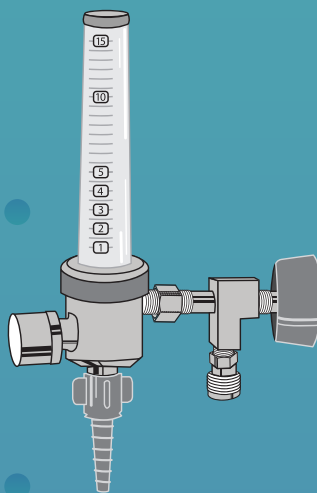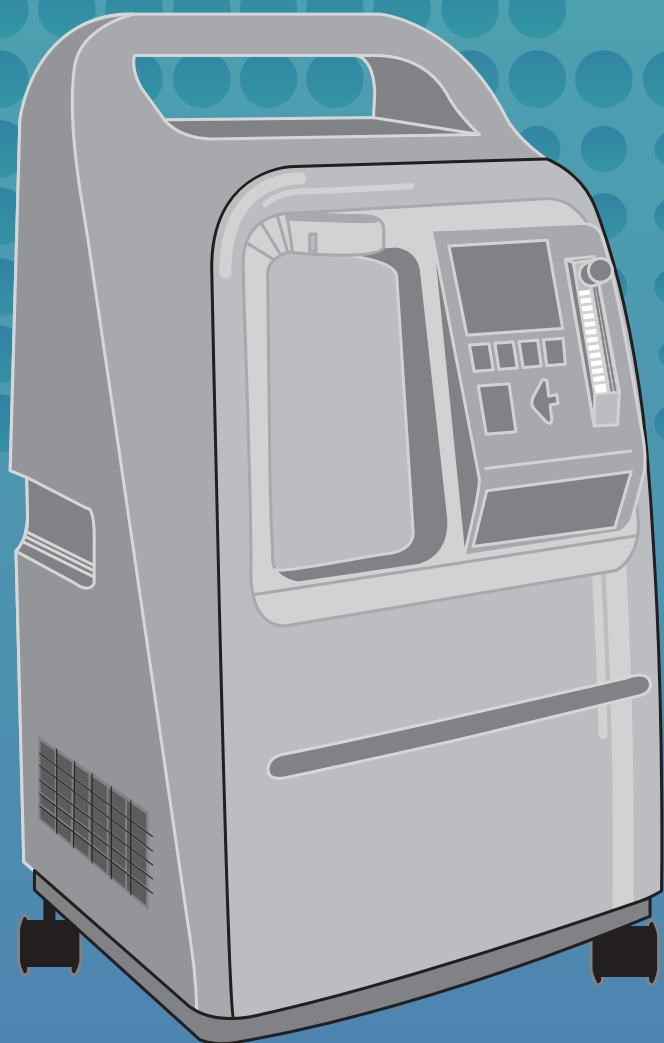



World Health
Organization



WHO-UNICEF TECHNICAL SPECIFICATIONS AND GUIDANCE FOR OXYGEN THERAPY DEVICES

WHO MEDICAL DEVICE TECHNICAL SERIES

WHO-UNICEF technical specifications and guidance for oxygen therapy devices

(WHO medical device technical series)

ISBN 978-92-4-151691-4 (WHO)

© **World Health Organization and the United Nations Children's Fund (UNICEF), 2019**

This joint report reflects the activities of the World Health Organization (WHO) and the United Nations Children's Fund (UNICEF)

Some rights reserved. This work is available under the Creative Commons Attribution-NonCommercial-ShareAlike 3.0 IGO licence (CC BY-NC-SA 3.0 IGO; <https://creativecommons.org/licenses/by-nc-sa/3.0/igo>).

Under the terms of this licence, you may copy, redistribute and adapt the work for non-commercial purposes, provided the work is appropriately cited, as indicated below. In any use of this work, there should be no suggestion that WHO or UNICEF endorses any specific organization, products or services. The unauthorized use of the WHO or UNICEF names or logos is not permitted. If you adapt the work, then you must license your work under the same or equivalent Creative Commons licence. If you create a translation of this work, you should add the following disclaimer along with the suggested citation: "This translation was not created by the World Health Organization (WHO) or the United Nations Children's Fund (UNICEF). Neither WHO nor UNICEF are responsible for the content or accuracy of this translation. The original English edition shall be the binding and authentic edition".

Any mediation relating to disputes arising under the licence shall be conducted in accordance with the mediation rules of the World Intellectual Property Organization (<http://www.wipo.int/amc/en/mediation/rules>).

Suggested citation. WHO-UNICEF technical specifications and guidance for oxygen therapy devices. Geneva: World Health Organization and the United Nations Children's Fund (UNICEF), 2019 (WHO medical device technical series). Licence: CC BY-NC-SA 3.0 IGO.

Cataloguing-in-Publication (CIP) data. CIP data are available at <http://apps.who.int/iris>.

Sales, rights and licensing. To purchase WHO publications, see <http://apps.who.int/bookorders>. To submit requests for commercial use and queries on rights and licensing, see <http://www.who.int/about/licensing>.

Third-party materials. If you wish to reuse material from this work that is attributed to a third party, such as tables, figures or images, it is your responsibility to determine whether permission is needed for that reuse and to obtain permission from the copyright holder. The risk of claims resulting from infringement of any third-party-owned component in the work rests solely with the user.

General disclaimers. The designations employed and the presentation of the material in this publication do not imply the expression of any opinion whatsoever on the part of WHO or UNICEF concerning the legal status of any country, territory, city or area or of its authorities, or concerning the delimitation of its frontiers or boundaries. Dotted and dashed lines on maps represent approximate border lines for which there may not yet be full agreement.

The mention of specific companies or of certain manufacturers' products does not imply that they are endorsed or recommended by WHO or UNICEF in preference to others of a similar nature that are not mentioned. Errors and omissions excepted, the names of proprietary products are distinguished by initial capital letters.

All reasonable precautions have been taken by WHO and UNICEF to verify the information contained in this publication. However, the published material is being distributed without warranty of any kind, either expressed or implied. The responsibility for the interpretation and use of the material lies with the reader. In no event shall WHO or UNICEF be liable for damages arising from its use.

Illustrations by Margot Steiner

Design and layout by L'IV Com Sàrl

Contents

Acknowledgements	v
Abbreviations	vii
Executive summary	viii
1 Introduction	2
1.1 Background	2
1.2 Purpose of the manual	3
1.3 How to read this document	4
1.4 Target audience	5
1.5 Development process	6
References	6
2 Overview of oxygen therapy products	10
2.1 Landscape of oxygen therapy products	10
2.2 Scope of this publication	13
Reference	13
3 Oxygen sources	16
3.1 Overview of different oxygen sources	16
3.2 Technical specifications for oxygen cylinders	21
3.3 Technical specifications for oxygen concentrators	25
References	25
4 Devices for oxygen regulation and conditioning	28
4.1 Overview of flowmeters	28
4.2 Technical specifications for Thorpe tube flowmeters	31
4.3 Overview of flow-splitting devices	34
4.4 Technical specifications for flowmeter stands	36
4.5 Overview of humidifiers	38
4.6 Technical specifications for reusable non-heated bubble humidifiers	39
References	42
5 Oxygen delivery devices	44
5.1 Overview of oxygen delivery devices	44
5.2 Technical specifications for nasal cannulae, nasal catheters and oxygen tubing	45
References	50
6 Pulse oximetry	52
6.1 Overview of pulse oximeters	52
6.2 Overview of pulse oximeter probes	55
6.3 Technical specifications for self-contained fingertip pulse oximeters	57
6.4 Technical specifications for handheld pulse oximeters	60
6.5 Technical specifications for tabletop pulse oximeters	63
References	65

7	Devices for quality power supply	68
7.1	Overview of devices for quality power supply	68
7.2	Technical specifications for solid-state voltage stabilizers	71
7.3	Technical specifications for surge suppressors	73
	References	75
8	Oxygen analysers	78
8.1	Overview of oxygen analysers	78
8.2	Technical specifications for electrochemical (galvanic cell) oxygen analysers	81
8.3	Technical specifications for ultrasonic oxygen analysers	83
	Reference	84
	Annex 1: Technical specifications for oxygen therapy devices	86
	Table A1.1: Technical specifications for oxygen cylinders	87
	Table A1.2: Technical specifications for oxygen concentrators	93
	Table A1.3: Technical specifications for Thorpe tube flowmeters	97
	Table A1.4: Technical specifications for flowmeter stands	101
	Table A1.5: Technical specifications for reusable non-heated bubble humidifiers	105
	Table A1.6: Technical specifications for nasal cannulae	109
	Table A1.7: Technical specifications for nasal catheters	113
	Table A1.8: Technical specifications for oxygen tubing	117
	Table A1.9: Technical specifications for self-contained fingertip pulse oximeters	121
	Table A1.10: Technical specifications for handheld pulse oximeters	125
	Table A1.11: Technical specifications for tabletop pulse oximeters	129
	Table A1.12: Technical specifications for solid-state voltage stabilizers	133
	Table A1.13: Technical specifications for surge suppressors	137
	Table A1.14: Technical specifications for electrochemical (galvanic cell) oxygen analysers	141
	Table A1.15: Technical specifications for ultrasonic oxygen analysers	145
	Annex 2: Comparison of pulse oximetry and blood gas analysis	149

Acknowledgements

The *WHO-UNICEF Technical specifications and guidance for oxygen therapy devices* publication has been developed by the United Nations Children's Fund (UNICEF) in collaboration with the World Health Organization (WHO) to help increase access to and utilization of life-saving oxygen therapy systems in low-resource settings.

Mulugeta Mideksa Amene and Beverly Bradley (Product Innovation Centre, UNICEF, Copenhagen, Denmark) drafted this document with input from Jonas Karlstrom (Product Innovation Centre, UNICEF) and Andrew Gammie (Fishtail Consulting Ltd, Chippenham, United Kingdom of Great Britain and Northern Ireland [United Kingdom]). Umberto Vitale (Product Innovation Centre, UNICEF) developed the first draft of the interagency technical specifications.

Adriana Velazquez Berumen (Senior advisor on medical devices, Essential Medicines and Health Products Department, WHO, Geneva, Switzerland) provided technical input during the preparation of this document and coordinated the input from the following WHO staff: Shamim Ahmad Qazi, Walter Johnson and Wilson Were; WHO consultant, Alejandra Velez; and interns, Joshua Daniel and Karen Kulp.

This document, and the broader WHO-UNICEF collaboration to improve access to and utilization of oxygen therapy systems, which began in 2017 and continues into 2019, has benefited from technical and strategic advice from two expert groups: the Technical Review Group (TRG) and the Advisory Committee (AC). The members of these committees are listed below. All committee members submitted a declaration of interest form.

Technical Review Group members: Roberto Ayala (CENETEC-Salud, Mexico City, Mexico), Audrey Battu (Clinton Health Access Initiative [CHAI], Boston, MA, United States of America), Jim Black (FREO2 Foundation Australia, Melbourne, Australia), Michael Dobson (University of Oxford, United Kingdom), Mike Eisenstein (PATH, Seattle, WA, United States of America), Adegoke G Falade (University of Ibadan, Nigeria), Martha Gartley (CHAI), Hamish Graham (University of Melbourne, Australia), Stephen Howie (University of Auckland, New Zealand), Fyezah Jehan (Aga Khan University, Karachi, Pakistan), Ameel Mohammad (National Health Systems Resource Centre, New Delhi, India), Valentino Mvanga (Ministry of Health and Social Welfare, Dar Es Salaam, United Republic of Tanzania), Susan Niermeyer (University of Colorado, Denver, CO, United States of America), Tayo Olaleye (CHAI), David Peel (Ashdown Consultants, Uckfield, United Kingdom), Shamim Ahmad Qazi (Department of Maternal, Newborn, Child and Adolescent Health, WHO, Geneva, Switzerland), Iain Wilson (Lifebox, London, United Kingdom), Anna Worm (Anna Worm Ltd, France).

Advisory Committee members: Trevor Duke (University of Melbourne, Australia), Mike English (KEMRI-Wellcome Trust, University of Oxford, United Kingdom), Amy Ginsburg (Save the Children, Seattle, WA, United States of America), Jessica Jones (Bill & Melinda Gates Foundation, Seattle, WA, United States of America), Sushil Kabra (All India Institute of Medical Sciences, New Delhi, India), Smita Kumar (United States Agency for International Development [USAID], Washington, DC, United States of America), Abadi Leul (Mekelle University, Tigray, Ethiopia), Kathy Mellor (BirthLink, Ickenham, United Kingdom), Bernard Olayo (Centre for Public Health and Development, Nairobi, Kenya), Kate Schroder (CHAI), Lisa Smith (PATH), Martin Weber (Child and Adolescent Health, WHO Regional Office for Europe, Copenhagen, Denmark).

The following individuals from the TRG and AC are gratefully acknowledged for their direct contribution in reviewing and commenting on the interagency specifications and/or drafts of the technical guidance document: Roberto Ayala, Audrey Battu, Jim Black, Michael Dobson, Trevor Duke, Adegoke G Falade, Martha Gartley, Stephen Howie, Fyezah Jehan, Jessica Jones, Abadi Leul, Ameel Mohammad, Kathy Mellor, Susan Niermeyer, Tayo Olaleye, David Peel, Shamim Ahmad Qazi, Kate Schroder, Lisa Smith, Martin Weber, Iain Wilson and Anna Worm.

In addition to the above committee members, the following individuals are also acknowledged for their input to the draft: Pawan Kumar (National Health Systems Resource Centre, New Delhi, India), Grace Irimu-Thinwa (University of Nairobi, Kenya), Annamarie Saarinen (Newborn Foundation, Washington, DC, United States of America), Michael Ruffo (PATH) and Cindy McWhorter (Product Innovation Centre, UNICEF).

Paul LaBarre and Kristoffer Gandrup-Marino (Product Innovation Centre, UNICEF), along with Abdallah Makhlof (Health Technology Centre, UNICEF), have been instrumental in providing leadership and guidance throughout the many stages of this project.

We would like to acknowledge Vivien Stone (Etchingham, United Kingdom) for assistance in editing and Margot Steiner (Morges, Switzerland) for the illustrations. Federica Gabellini (Product Innovation Centre, UNICEF) is acknowledged for her communications coordination and support throughout the development of this publication.

Funding for this project was provided by the Bill & Melinda Gates Foundation.



预览已结束，完整报告链接和二维码如下：

https://www.yunbaogao.cn/report/index/report?reportId=5_25407

